

SWISSFLEX e y e w e a r

like wearing nothing.



perfect fit modular individuality 100% swiss-made



the better glasses fit, the better you see and feel!


Fitting components (nose, head, ear)

- · All available parts in all available colors
- · Identification of model and boxing size
- Mounting and demounting of temples
- Mounting and demounting of nosepads

Fitting System for nose



Modular ergonomic pads ensure best wearing comfort for each model and every face.

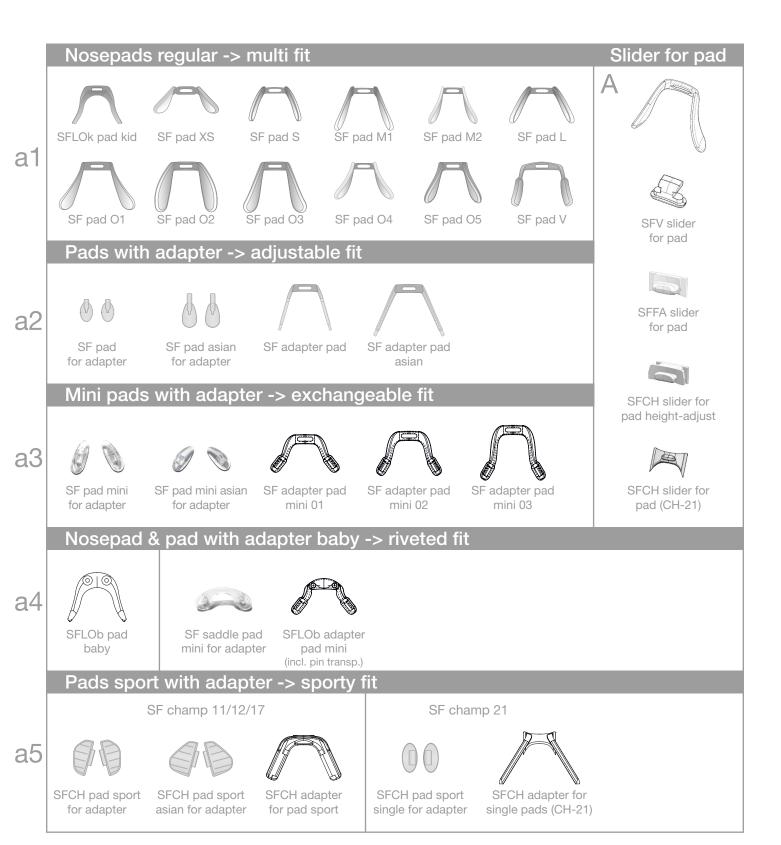

Fitting System for head and ears



Modular ergonomic endpieces ensure best wearing comfort for each model and every face.

	Model Systems	Temples	Endpieces			
				Sti	ck	
b1	all models but SFLOb	straight	SFC endpiece straight stick (fits SFC, SFCC, SFCk, SFCkC, SFLO, SFLOk, SFE, SFV)	SFAL endpiece straight stick (fits SFAL)	SFR endpiece straight stick (fits SFR, SFM)	
			1.1	1.2	1.3	
			Hook		Curved	Stick
b2	SF classic Contur SF classic Kid SF classic Kid Contur	raster	SFC endpiece raster hook	SFC endpiece raster hook strong	SFC endpiece raster curved	
	SF varius SF loop SF loop Kid		SFC endpiece raster hook kid	SFLOk endpiece raster hook gap		
			2.3	2.4		
b3	SF airlight	raster	SFAL endpiece raster hook			
			3.1			
b4	SF eyephorics	raster	SFE endpiece raster hook medium	SFE endpiece raster hook large	SFE endpiece raster curved	
			4.1	4.2	4.3	
b5	SF rainbow SF motion	raster	SFR endpiece raster hook	SFR endpiece raster hook heavy	SFR endpiece raster curved	SFR endpiece raster stick
	SF champ 21		5.1	5.2	5.3	5.4
b6	SF fashion	raster	SFFA endpiece raster hook			
			6.1			
	SF loop Baby	one piece frame	SFLOb endpiece raster hook	SFLOb endpiece raster hook gap		
b7			7.1	7.2		


Identification of Model and Boxing Size



The fronts (only boxing size), temples, nosepads, earpieces bear specific identifications. model model SFC, SFE, SFAL **SFM** ocular mode boxing size model boxing size model (on hinge under temple) (on hinge under temple) model model SFV **SFR SFFA**

Identification of Model and Boxing Size



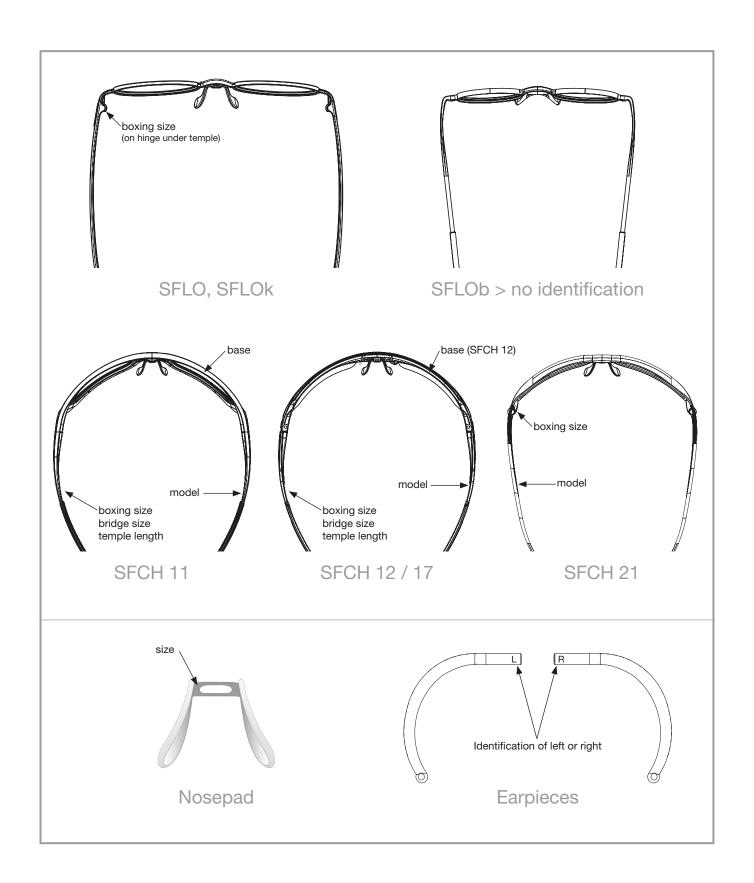

Mounting & Demounting of Temples (for Opticians only)



General


Click-out


- 1. Check always opening direction of hinge
- 2. Hold frame at a vertical angle
- 3. Secure hinge firmly with finger
- 4. Remove temple with a jolt off the hinge or lever the temple off the hinge (mind opening angle!)


Click-in


- 1. Check always opening direction of hinge
- 2. Secure hinge firmly with finger
- 3. Click in the temple with light pressure


Methods














Particularities and Tips

- · Mounting and demounting of temples is strong on purpose and serves the tight hold
- Protection of overexpansion for models SF loop, SF loop Kid, SF champ
- · Removing temple with a jolt is important, otherwise the material can be overexpanded
- Older hinges may vary please check opening direction of hinge
- · Demonstration videos are provided in the login-area of our homepage

Mounting and demounting of temples should be performed by trained opticians only, not by end consumers.

Nose Pads / Mounting & Demounting (for Opticians only)



Nose Pads (all except SF varius)

Tightly clicking the nose pads in and out is necessary to ensure a tight fit on the center section.



Assembly (with tool)

- 1. Place nose pad (wings downwards)
- 2. Press with wedge into slot
- 3. Place center part with mushroom facing down on top of wedge
- 4. Press center part down vertically until nose pad clicks into place



Disassembly (without tool)

- Position middle part with nose pad inwards & downwards
- 2. Place thumb on lower part of ,wings'
- 3. Press ,wings' with both thumbs simultaneously between glasses

Nose Pads for SF varius

The nosepad is connected to the front with the slider - not with the regular ,mushroom'.

1. Slider System



The nose pad including the slider can be easily pushed in or out with the thumb.

2. Mounting Slider to nosepad



1. The handle simplifies the insertion of the slider.



2. Insert the ,hook' through the wings in the hole.



3. Ensure proper click-in of slider.



4. Turn the handle to detach it from the slider.

Note

- If handled correctly, the nose pad will not be damaged, when clicked in and out.
- · Intentionally tight clicking in and out for a better grip.

